

CERTIFICATE OF ANALYSIS

REPORTED TO Alana Lins (Salmo, Village of)
Box 1000
Salmo, BC V0G 1Z0

ONLINE ORDER# 485250

SITE INFO Online Order #485250
CARO WO# 22D0861

RECEIVED / TEMP 2022-04-13 09:15 / 3.6°C
REPORTED 2022-04-25

Introduction:

CARO Analytical Services is a testing laboratory full of smart, engaged scientists driven to make the world a safer and healthier place. Through our clients' projects we become an essential element for a better world. We employ methods conducted in accordance with recognized professional standards using accepted testing methodologies and quality control efforts. CARO is accredited by the Canadian Association for Laboratories Accreditation (CALA) to ISO/IEC 17025:2017 for specific tests listed in the scope of accreditation approved by CALA.

Big Picture Sidekicks



You know that the sample you collected after snowshoeing to site, digging 5 meters, and racing to get it on a plane so you can submit it to the lab for time sensitive results needed to make important and expensive decisions (whew) is VERY important. We know that too.

We've Got Chemistry



It's simple. We figure the more you enjoy working with our fun and engaged team members; the more likely you are to give us continued opportunities to support you.

Ahead of the Curve



Through research, regulation knowledge, and instrumentation, we are your analytical centre for the technical knowledge you need, BEFORE you need it, so you can stay up to date and in the know.

Report Highlights:

The results in this report apply to the samples analyzed in accordance with your submission. All parameters meet the Guidelines for Canadian Drinking Water Quality (Jan 2020).

For more information, please visit <http://www.caro.ca/reports/>

Laboratory Recommendations:

For assistance interpreting your results, please visit

www.caro.ca/you-need-to-know-about-bacteria-in-water-analytical-report/


Regular testing of your water is recommended to ensure ongoing suitability for use; we recommend at least yearly. Please visit <https://www.caro.ca/store> for a list of CARO's testing packages. If you have any additional questions or concerns, please contact us at teamcaro@caro.ca.

Authorized By:

Team CARO
Client Service Representative

1-888-311-8846 | www.caro.ca

#110 4011 Viking Way Richmond, BC V6V 2K9 | #102 3677 Highway 97N Kelowna, BC V1X 5C3 | 17225 109 Avenue Edmonton, AB T5S 1H7 |
#108 4475 Wayburne Drive Burnaby, BC V5G 4X4

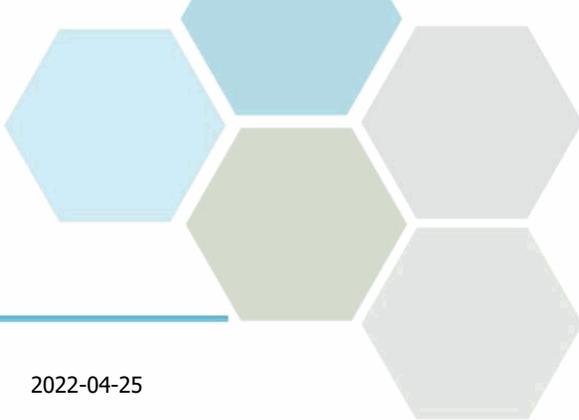

TEST RESULTS

REPORTED TO Alana Lins (Salmo, Village of)
CARO WO# 22D0861

REPORTED 2022-04-25

Parameter	Result	Guideline	RL Units	Analyzed	Note
Sample Name: Lagoon Road, Salmo Matrix: Water Sampled: 2022-04-12 13:00					
Anions					
Chloride	2.49	AO ≤ 250	0.10 mg/L	2022-04-15	
Fluoride	< 0.10	MAC = 1.5	0.10 mg/L	2022-04-15	
Nitrate (as N)	0.092	MAC = 10	0.010 mg/L	2022-04-15	
Nitrite (as N)	< 0.010	MAC = 1	0.010 mg/L	2022-04-15	
Sulfate	12.7	AO ≤ 500	1.0 mg/L	2022-04-15	
Calculated Parameters					
Hardness, Total (as CaCO3)	90.2	None Required	0.500 mg/L	N/A	
Solids, Total Dissolved	111	AO ≤ 500	1.00 mg/L	N/A	
General Parameters					
Alkalinity, Total (as CaCO3)	92.7	N/A	1.0 mg/L	2022-04-21	
Conductivity (EC)	193	N/A	2.0 µS/cm	2022-04-21	
Cyanide, Total	< 0.0020	MAC = 0.2	0.0020 mg/L	2022-04-20	
pH	7.78	7.0-10.5	0.10 pH units	2022-04-21	HT2
Turbidity	0.16	OG < 1	0.10 NTU	2022-04-14	
Microbiological Parameters					
Coliforms, Total	< 1	MAC = 0	1 CFU/100 mL	2022-04-13	
E. coli	< 1	MAC = 0	1 CFU/100 mL	2022-04-13	
Total Metals					
Aluminum, total	< 0.0050	OG < 0.1	0.0050 mg/L	2022-04-19	
Antimony, total	< 0.00020	MAC = 0.006	0.00020 mg/L	2022-04-19	
Arsenic, total	< 0.00050	MAC = 0.01	0.00050 mg/L	2022-04-19	
Barium, total	0.0232	MAC = 2	0.0050 mg/L	2022-04-19	
Boron, total	< 0.0500	MAC = 5	0.0500 mg/L	2022-04-19	
Cadmium, total	0.000021	MAC = 0.005	0.000010 mg/L	2022-04-19	
Calcium, total	30.7	None Required	0.20 mg/L	2022-04-19	
Chromium, total	0.00090	MAC = 0.05	0.00050 mg/L	2022-04-19	
Copper, total	0.00743	MAC = 2	0.00040 mg/L	2022-04-19	
Iron, total	< 0.010	AO ≤ 0.3	0.010 mg/L	2022-04-19	
Lead, total	0.00028	MAC = 0.005	0.00020 mg/L	2022-04-19	
Magnesium, total	3.24	None Required	0.010 mg/L	2022-04-19	
Manganese, total	< 0.00020	MAC = 0.12	0.00020 mg/L	2022-04-19	
Potassium, total	1.48	N/A	0.10 mg/L	2022-04-19	
Selenium, total	0.00075	MAC = 0.05	0.00050 mg/L	2022-04-19	
Sodium, total	2.95	AO ≤ 200	0.10 mg/L	2022-04-19	
Strontium, total	0.160	MAC = 7	0.0010 mg/L	2022-04-19	
Uranium, total	0.000979	MAC = 0.02	0.000020 mg/L	2022-04-19	
Zinc, total	0.0063	AO ≤ 5	0.0040 mg/L	2022-04-19	

Note Descriptions:

HT2 The 15 minute recommended holding time (from sampling to analysis) has been exceeded - field analysis is recommended.

APPENDIX 1: SUPPORTING INFORMATION

REPORTED TO Alana Lins (Salmo, Village of)
CARO WO# 22D0861


REPORTED 2022-04-25

Analysis Description	Method Ref.	Technique	Accredited	Location
Alkalinity in Water	SM 2320 B* (2017)	Titration with H2SO4	✓	Kelowna
Anions in Water	SM 4110 B (2017)	Ion Chromatography	✓	Kelowna
Coliforms, Total in Water	SM 9222* (2017)	Membrane Filtration / Chromocult Agar	✓	Kelowna
Conductivity in Water	SM 2510 B (2017)	Conductivity Meter	✓	Kelowna
Cyanide, SAD in Water	ASTM D7511-12	Flow Injection with In-Line UV Digestion and Amperometry	✓	Kelowna
E. coli in Water	SM 9222* (2017)	Membrane Filtration / Chromocult Agar	✓	Kelowna
Hardness in Water	SM 2340 B* (2017)	Calculation: 2.497 [total Ca] + 4.118 [total Mg] (Est)	✓	N/A
pH in Water	SM 4500-H+ B (2017)	Electrometry	✓	Kelowna
Solids, Total Dissolved in Water	SM 1030 E (2017)	SM 1030 E (2011)		N/A
Total Metals in Water	EPA 200.2 / EPA 6020B	HNO3+HCl Hot Block Digestion / Inductively Coupled Plasma-Mass Spectroscopy (ICP-MS)	✓	Richmond
Turbidity in Water	SM 2130 B (2017)	Nephelometry	✓	Kelowna

Note: An asterisk in the Method Reference indicates that the CARO method has been modified from the reference method

Glossary:

RL	Reporting Limit (default)
<	Less than the specified Reporting Limit (RL) - the actual RL may be higher than the default RL due to various factors
AO	Aesthetic Objective
CFU/100 mL	Colony Forming Units per 100 millilitres
MAC	Maximum Acceptable Concentration (health based)
mg/L	Milligrams per litre
NTU	Nephelometric Turbidity Units
OG	Operational Guideline (treated water)
pH units	pH < 7 = acidic, pH > 7 = basic
µS/cm	Microsiemens per centimetre
ASTM	ASTM International Test Methods
EPA	United States Environmental Protection Agency Test Methods
SM	Standard Methods for the Examination of Water and Wastewater, American Public Health Association

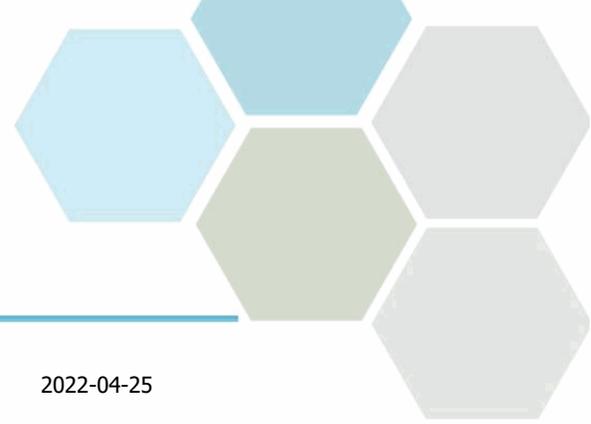

APPENDIX 1: SUPPORTING INFORMATION

REPORTED TO Alana Lins (Salmo, Village of)
CARO WO# 22D0861

REPORTED 2022-04-25


General Comments:

For assistance interpreting your results, please visit
www.caro.ca/you-need-to-know-about-bacteria-in-water-analytical-report/

The results in this report apply to the samples analyzed in accordance with the Chain of Custody document. This analytical report must be reproduced in its entirety. CARO is not responsible for any loss or damage resulting directly or indirectly from error or omission in the conduct of testing. Liability is limited to the cost of analysis. Samples will be disposed of 30 days after the test report has been issued or once samples expire, whichever comes first. Longer hold is possible if agreed to in writing.

Results in **Bold** indicate values that are above CARO's method reporting limits. Any results that are above regulatory limits are highlighted **red**. Please note that results will only be highlighted red if the regulatory limits are included on the CARO report. Any Bold and/or highlighted results do not take into account method uncertainty. If you would like method uncertainty or regulatory limits to be included on your report, please contact your Account Manager: teamcaro@caro.ca

Please note any regulatory guidelines applied to this report are added as a convenience to the client, at their request, to help provide some initial context to analytical results obtained. Although CARO makes every effort to ensure accuracy of the associated regulatory guideline(s) applied, the guidelines applied cannot be assumed to be correct due to a variety of factors and as such CARO Analytical Services assumes no liability or responsibility for the use of those guidelines to make any decisions. The original source of the regulation should be verified and a review of the guideline(s) should be validated as correct in order to make any decisions arising from the comparison of the analytical data obtained to the relevant regulatory guideline for one's particular circumstances. Further, CARO Analytical Services assumes no liability or responsibility for any loss attributed from the use of these guidelines in any way.

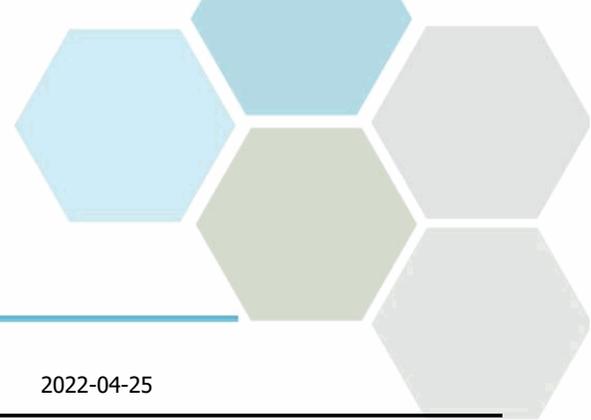

APPENDIX 2: QUALITY CONTROL RESULTS

REPORTED TO Alana Lins (Salmo, Village of)
CARO WO# 22D0861


REPORTED 2022-04-25

The following section displays the quality control (QC) data that is associated with your sample data. Groups of samples are prepared in "batches" and analyzed in conjunction with QC samples that ensure your data is of the highest quality. Common QC types include:

- **Method Blank (Blk):** A blank sample that undergoes sample processing identical to that carried out for the test samples. Method blank results are used to assess contamination from the laboratory environment and reagents.
- **Duplicate (Dup):** An additional or second portion of a randomly selected sample in the analytical run carried through the entire analytical process. Duplicates provide a measure of the analytical method's precision (reproducibility).
- **Blank Spike (BS):** A sample of known concentration which undergoes processing identical to that carried out for test samples, also referred to as a laboratory control sample (LCS). Blank spikes provide a measure of the analytical method's accuracy.
- **Matrix Spike (MS):** A second aliquot of sample is fortified with a known concentration of target analytes and carried through the entire analytical process. Matrix spikes evaluate potential matrix effects that may affect the analyte recovery.
- **Reference Material (SRM):** A homogenous material of similar matrix to the samples, certified for the parameter(s) listed. Reference Materials ensure that the analytical process is adequate to achieve acceptable recoveries of the parameter(s) tested.

Each QC type is analyzed at a 5-10% frequency, i.e. one blank/duplicate/spike for every 10-20 samples. For all types of QC, the specified recovery (% Rec) and relative percent difference (RPD) limits are derived from long-term method performance averages and/or prescribed by the reference method.

Analyte	Result	MRL Units	Spike Level	Source Result	% REC	REC Limit	% RPD	RPD Limit	Notes
Anions, Batch B2D1291									
Blank (B2D1291-BLK1)			Prepared: 2022-04-15, Analyzed: 2022-04-15						
Chloride	< 0.10	0.10 mg/L							
Fluoride	< 0.10	0.10 mg/L							
Nitrate (as N)	< 0.010	0.010 mg/L							
Nitrite (as N)	< 0.010	0.010 mg/L							
Sulfate	< 0.5	0.5 mg/L							
Blank (B2D1291-BLK2)			Prepared: 2022-04-15, Analyzed: 2022-04-15						
Chloride	< 0.10	0.10 mg/L							
Fluoride	< 0.10	0.10 mg/L							
Nitrate (as N)	< 0.010	0.010 mg/L							
Nitrite (as N)	< 0.010	0.010 mg/L							
Sulfate	< 0.5	0.5 mg/L							
Blank (B2D1291-BLK3)			Prepared: 2022-04-15, Analyzed: 2022-04-15						
Chloride	< 0.10	0.10 mg/L							
Fluoride	< 0.10	0.10 mg/L							
Nitrate (as N)	< 0.010	0.010 mg/L							
Nitrite (as N)	< 0.010	0.010 mg/L							
Sulfate	< 0.5	0.5 mg/L							
LCS (B2D1291-BS1)			Prepared: 2022-04-15, Analyzed: 2022-04-15						
Chloride	15.9	0.10 mg/L	16.0		99	90-110			
Fluoride	3.96	0.10 mg/L	4.00		99	88-108			
Nitrate (as N)	3.89	0.010 mg/L	4.00		97	90-110			
Nitrite (as N)	1.95	0.010 mg/L	2.00		98	85-115			
Sulfate	15.7	0.5 mg/L	16.0		98	90-110			
LCS (B2D1291-BS2)			Prepared: 2022-04-15, Analyzed: 2022-04-15						
Chloride	15.6	0.10 mg/L	16.0		97	90-110			
Fluoride	4.06	0.10 mg/L	4.00		101	88-108			
Nitrate (as N)	3.89	0.010 mg/L	4.00		97	90-110			
Nitrite (as N)	1.91	0.010 mg/L	2.00		96	85-115			
Sulfate	15.8	0.5 mg/L	16.0		99	90-110			
LCS (B2D1291-BS3)			Prepared: 2022-04-15, Analyzed: 2022-04-15						
Chloride	15.6	0.10 mg/L	16.0		97	90-110			

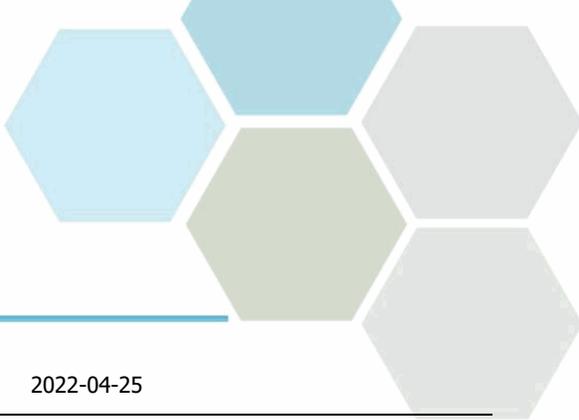

APPENDIX 2: QUALITY CONTROL RESULTS

REPORTED TO Alana Lins (Salmo, Village of)
CARO WO# 22D0861

REPORTED 2022-04-25

Analyte	Result	MRL Units	Spike Level	Source Result	% REC	REC Limit	% RPD	RPD Limit	Notes
Anions, Batch B2D1291, Continued									
LCS (B2D1291-BS3), Continued			Prepared: 2022-04-15, Analyzed: 2022-04-15						
Fluoride	3.92	0.10 mg/L	4.00		98	88-108			
Nitrate (as N)	3.89	0.010 mg/L	4.00		97	90-110			
Nitrite (as N)	1.92	0.010 mg/L	2.00		96	85-115			
Sulfate	15.8	0.5 mg/L	16.0		99	90-110			

General Parameters, Batch B2D1510

Blank (B2D1510-BLK1)			Prepared: 2022-04-14, Analyzed: 2022-04-14						
Turbidity	< 0.10	0.10 NTU							
Blank (B2D1510-BLK2)			Prepared: 2022-04-14, Analyzed: 2022-04-14						
Turbidity	< 0.10	0.10 NTU							
LCS (B2D1510-BS1)			Prepared: 2022-04-14, Analyzed: 2022-04-14						
Turbidity	39.8	0.10 NTU	40.0		100	90-110			
LCS (B2D1510-BS2)			Prepared: 2022-04-14, Analyzed: 2022-04-14						
Turbidity	38.7	0.10 NTU	40.0		97	90-110			

General Parameters, Batch B2D1810

Blank (B2D1810-BLK1)			Prepared: 2022-04-20, Analyzed: 2022-04-20						
Cyanide, Total	< 0.0020	0.0020 mg/L							
Blank (B2D1810-BLK2)			Prepared: 2022-04-20, Analyzed: 2022-04-20						
Cyanide, Total	< 0.0020	0.0020 mg/L							
LCS (B2D1810-BS1)			Prepared: 2022-04-20, Analyzed: 2022-04-20						
Cyanide, Total	0.0199	0.0020 mg/L	0.0200		99	82-120			
LCS (B2D1810-BS2)			Prepared: 2022-04-20, Analyzed: 2022-04-20						
Cyanide, Total	0.0198	0.0020 mg/L	0.0200		99	82-120			
LCS Dup (B2D1810-BSD1)			Prepared: 2022-04-20, Analyzed: 2022-04-20						
Cyanide, Total	0.0195	0.0020 mg/L	0.0200		98	82-120	2	10	
LCS Dup (B2D1810-BSD2)			Prepared: 2022-04-20, Analyzed: 2022-04-20						
Cyanide, Total	0.0198	0.0020 mg/L	0.0200		99	82-120	< 1	10	
Matrix Spike (B2D1810-MS1)			Source: 22D0861-01			Prepared: 2022-04-20, Analyzed: 2022-04-20			
Cyanide, Total	0.0400	0.0020 mg/L	0.0400	< 0.0020	100	70-130			

General Parameters, Batch B2D1997

Blank (B2D1997-BLK1)			Prepared: 2022-04-21, Analyzed: 2022-04-21						
Alkalinity, Total (as CaCO3)	< 1.0	1.0 mg/L							
Alkalinity, Phenolphthalein (as CaCO3)	< 1.0	1.0 mg/L							
Alkalinity, Bicarbonate (as CaCO3)	< 1.0	1.0 mg/L							
Alkalinity, Carbonate (as CaCO3)	< 1.0	1.0 mg/L							
Alkalinity, Hydroxide (as CaCO3)	< 1.0	1.0 mg/L							
Conductivity (EC)	< 2.0	2.0 µS/cm							
Blank (B2D1997-BLK2)			Prepared: 2022-04-21, Analyzed: 2022-04-21						
Alkalinity, Total (as CaCO3)	< 1.0	1.0 mg/L							
Alkalinity, Phenolphthalein (as CaCO3)	< 1.0	1.0 mg/L							
Alkalinity, Bicarbonate (as CaCO3)	< 1.0	1.0 mg/L							



APPENDIX 2: QUALITY CONTROL RESULTS

REPORTED TO Alana Lins (Salmo, Village of)
CARO WO# 22D0861

REPORTED 2022-04-25

Analyte	Result	MRL Units	Spike Level	Source Result	% REC	REC Limit	% RPD	RPD Limit	Notes
General Parameters, Batch B2D1997, Continued									
Blank (B2D1997-BLK2), Continued			Prepared: 2022-04-21, Analyzed: 2022-04-21						
Alkalinity, Carbonate (as CaCO ₃)	< 1.0	1.0 mg/L							
Alkalinity, Hydroxide (as CaCO ₃)	< 1.0	1.0 mg/L							
Conductivity (EC)	< 2.0	2.0 µS/cm							
LCS (B2D1997-BS1)			Prepared: 2022-04-21, Analyzed: 2022-04-21						
Alkalinity, Total (as CaCO ₃)	105	1.0 mg/L	100		105	80-120			
LCS (B2D1997-BS2)			Prepared: 2022-04-21, Analyzed: 2022-04-21						
Alkalinity, Total (as CaCO ₃)	109	1.0 mg/L	100		109	80-120			
LCS (B2D1997-BS3)			Prepared: 2022-04-21, Analyzed: 2022-04-21						
Conductivity (EC)	1430	2.0 µS/cm	1410		101	95-105			
LCS (B2D1997-BS4)			Prepared: 2022-04-21, Analyzed: 2022-04-21						
Conductivity (EC)	1420	2.0 µS/cm	1410		101	95-105			
Reference (B2D1997-SRM1)			Prepared: 2022-04-21, Analyzed: 2022-04-21						
pH	7.02	0.10 pH units	7.01		100	98-102			
Reference (B2D1997-SRM2)			Prepared: 2022-04-21, Analyzed: 2022-04-21						
pH	7.02	0.10 pH units	7.01		100	98-102			

Microbiological Parameters, Batch B2D1347

Blank (B2D1347-BLK1)			Prepared: 2022-04-13, Analyzed: 2022-04-13						
Coliforms, Total	< 1	1 CFU/100 mL							
E. coli	< 1	1 CFU/100 mL							
Blank (B2D1347-BLK2)			Prepared: 2022-04-13, Analyzed: 2022-04-13						
Coliforms, Total	< 1	1 CFU/100 mL							
E. coli	< 1	1 CFU/100 mL							
Blank (B2D1347-BLK3)			Prepared: 2022-04-13, Analyzed: 2022-04-13						
Coliforms, Total	< 1	1 CFU/100 mL							
E. coli	< 1	1 CFU/100 mL							
Blank (B2D1347-BLK4)			Prepared: 2022-04-13, Analyzed: 2022-04-13						
Coliforms, Total	< 1	1 CFU/100 mL							
E. coli	< 1	1 CFU/100 mL							
Blank (B2D1347-BLK5)			Prepared: 2022-04-13, Analyzed: 2022-04-13						
Coliforms, Total	< 1	1 CFU/100 mL							
E. coli	< 1	1 CFU/100 mL							
Blank (B2D1347-BLK6)			Prepared: 2022-04-13, Analyzed: 2022-04-13						
Coliforms, Total	< 1	1 CFU/100 mL							
E. coli	< 1	1 CFU/100 mL							
Blank (B2D1347-BLK7)			Prepared: 2022-04-13, Analyzed: 2022-04-13						
Coliforms, Total	< 1	1 CFU/100 mL							
E. coli	< 1	1 CFU/100 mL							
Blank (B2D1347-BLK8)			Prepared: 2022-04-13, Analyzed: 2022-04-13						
Coliforms, Total	< 1	1 CFU/100 mL							
E. coli	< 1	1 CFU/100 mL							
Blank (B2D1347-BLK9)			Prepared: 2022-04-13, Analyzed: 2022-04-13						
Coliforms, Total	< 1	1 CFU/100 mL							




APPENDIX 2: QUALITY CONTROL RESULTS

REPORTED TO Alana Lins (Salmo, Village of)
CARO WO# 22D0861

REPORTED 2022-04-25

Analyte	Result	MRL Units	Spike Level	Source Result	% REC	REC Limit	% RPD	RPD Limit	Notes
Microbiological Parameters, Batch B2D1347, Continued									
Blank (B2D1347-BLK9), Continued					Prepared: 2022-04-13, Analyzed: 2022-04-13				
E. coli	< 1	1 CFU/100 mL							
Blank (B2D1347-BLKA)					Prepared: 2022-04-13, Analyzed: 2022-04-13				
Coliforms, Total	< 1	1 CFU/100 mL							
E. coli	< 1	1 CFU/100 mL							
Blank (B2D1347-BLKB)					Prepared: 2022-04-13, Analyzed: 2022-04-13				
Coliforms, Total	< 1	1 CFU/100 mL							
E. coli	< 1	1 CFU/100 mL							
Blank (B2D1347-BLKC)					Prepared: 2022-04-13, Analyzed: 2022-04-13				
Coliforms, Total	< 1	1 CFU/100 mL							
E. coli	< 1	1 CFU/100 mL							
Total Metals, Batch B2D1651									
Blank (B2D1651-BLK1)					Prepared: 2022-04-19, Analyzed: 2022-04-19				
Aluminum, total	< 0.0050	0.0050 mg/L							
Antimony, total	< 0.00020	0.00020 mg/L							
Arsenic, total	< 0.00050	0.00050 mg/L							
Barium, total	< 0.0050	0.0050 mg/L							
Boron, total	< 0.0500	0.0500 mg/L							
Cadmium, total	< 0.000010	0.000010 mg/L							
Calcium, total	< 0.20	0.20 mg/L							
Chromium, total	< 0.00050	0.00050 mg/L							
Copper, total	< 0.00040	0.00040 mg/L							
Iron, total	< 0.010	0.010 mg/L							
Lead, total	< 0.00020	0.00020 mg/L							
Magnesium, total	< 0.010	0.010 mg/L							
Manganese, total	< 0.00020	0.00020 mg/L							
Potassium, total	< 0.10	0.10 mg/L							
Selenium, total	< 0.00050	0.00050 mg/L							
Sodium, total	< 0.10	0.10 mg/L							
Strontium, total	< 0.0010	0.0010 mg/L							
Uranium, total	0.000027	0.000020 mg/L							BLK
Zinc, total	< 0.0040	0.0040 mg/L							
LCS (B2D1651-BS1)					Prepared: 2022-04-19, Analyzed: 2022-04-19				
Aluminum, total	0.0223	0.0050 mg/L	0.0200		112	80-120			
Antimony, total	0.0211	0.00020 mg/L	0.0200		106	80-120			
Arsenic, total	0.0212	0.00050 mg/L	0.0200		106	80-120			
Barium, total	0.0218	0.0050 mg/L	0.0200		109	80-120			
Boron, total	< 0.0500	0.0500 mg/L	0.0200		101	80-120			
Cadmium, total	0.0209	0.000010 mg/L	0.0200		105	80-120			
Calcium, total	1.99	0.20 mg/L	2.00		100	80-120			
Chromium, total	0.0211	0.00050 mg/L	0.0200		106	80-120			
Copper, total	0.0212	0.00040 mg/L	0.0200		106	80-120			
Iron, total	2.06	0.010 mg/L	2.00		103	80-120			
Lead, total	0.0188	0.00020 mg/L	0.0200		94	80-120			
Magnesium, total	2.15	0.010 mg/L	2.00		107	80-120			
Manganese, total	0.0209	0.00020 mg/L	0.0200		105	80-120			
Potassium, total	2.13	0.10 mg/L	2.00		106	80-120			
Selenium, total	0.0205	0.00050 mg/L	0.0200		103	80-120			
Sodium, total	2.13	0.10 mg/L	2.00		107	80-120			
Strontium, total	0.0208	0.0010 mg/L	0.0200		104	80-120			
Uranium, total	0.0203	0.000020 mg/L	0.0200		101	80-120			

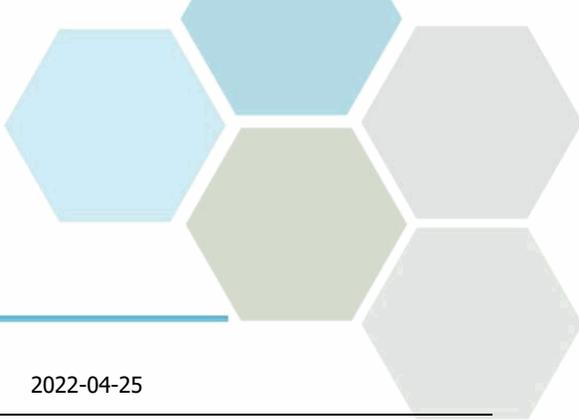

APPENDIX 2: QUALITY CONTROL RESULTS

REPORTED TO Alana Lins (Salmo, Village of)
CARO WO# 22D0861

REPORTED 2022-04-25

Analyte	Result	MRL Units	Spike Level	Source Result	% REC	REC Limit	% RPD	RPD Limit	Notes
Total Metals, Batch B2D1651, Continued									
LCS (B2D1651-BS1), Continued					Prepared: 2022-04-19, Analyzed: 2022-04-19				
Zinc, total	0.0210	0.0040 mg/L	0.0200		105	80-120			
Reference (B2D1651-SRM1)					Prepared: 2022-04-19, Analyzed: 2022-04-19				
Aluminum, total	0.216	0.0050 mg/L	0.198		109	70-130			
Antimony, total	0.0240	0.00020 mg/L	0.0230		104	70-130			
Arsenic, total	0.0218	0.00050 mg/L	0.0200		109	70-130			
Barium, total	0.0160	0.0050 mg/L	0.0161		100	70-130			
Boron, total	0.179	0.0500 mg/L	0.191		94	70-130			
Cadmium, total	0.00399	0.000010 mg/L	0.00404		99	70-130			
Calcium, total	0.87	0.20 mg/L	0.938		93	70-130			
Chromium, total	0.0268	0.00050 mg/L	0.0256		105	70-130			
Copper, total	0.0354	0.00040 mg/L	0.0322		110	70-130			
Iron, total	0.057	0.010 mg/L	0.0580		98	70-130			
Lead, total	0.00744	0.00020 mg/L	0.00796		93	70-130			
Magnesium, total	0.115	0.010 mg/L	0.112		103	70-130			
Manganese, total	0.0124	0.00020 mg/L	0.0120		103	70-130			
Potassium, total	0.87	0.10 mg/L	0.820		106	70-130			
Selenium, total	0.117	0.00050 mg/L	0.117		100	70-130			
Sodium, total	0.57	0.10 mg/L	0.490		116	70-130			
Strontium, total	0.295	0.0010 mg/L	0.276		107	70-130			
Uranium, total	0.00964	0.000020 mg/L	0.00970		99	70-130			
Zinc, total	0.0943	0.0040 mg/L	0.0884		107	70-130			

QC Qualifiers:

BLK Analyte concentration in the Method Blank is above the Reporting Limit (RL).